


# The meriT-1 Study

## Study Highlights

- Principal Investigator: Dr. Sameer Dani
- The meriT-1 was a single center, first-in-man trial which showed favourable results of BioMime sirolimus-eluting coronary stent system (SES) in treatment of *de novo* coronary artery lesions.
- Two years clinical follow-up with angiographic analysis at 8 months.

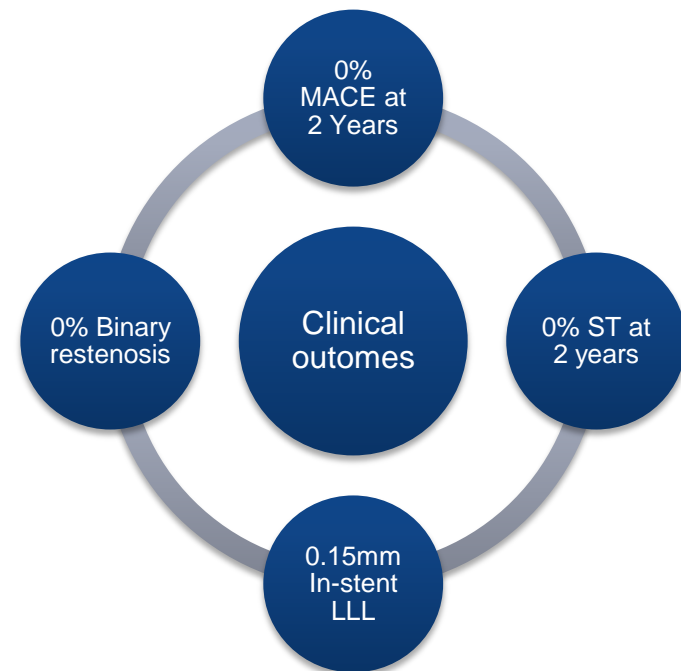

## ❖ Study Design

A prospective, non-randomized, single-arm, first-in-man trial



30 patients were enrolled





Angiographic follow-up at 8 months

Analysed by Cardiovascular Research Centre, Sao Paulo, Brazil



Clinical follow-up at 12 months and 24 months

❖ Study Results

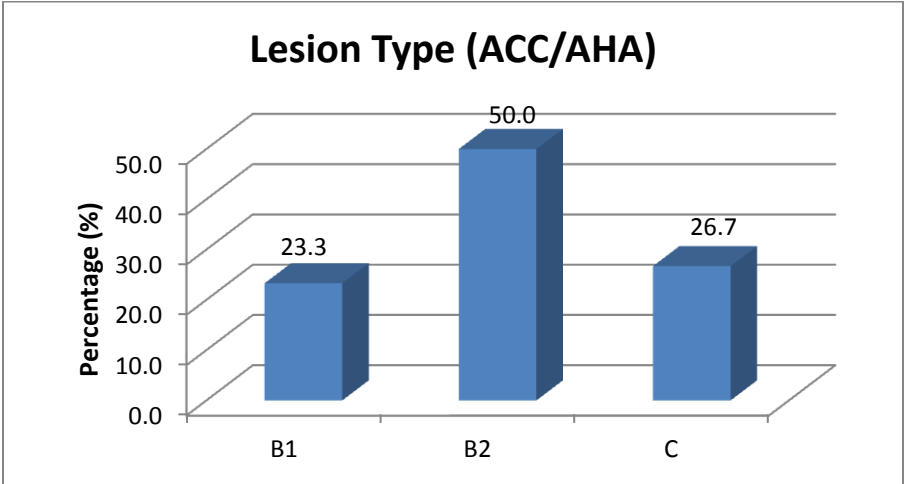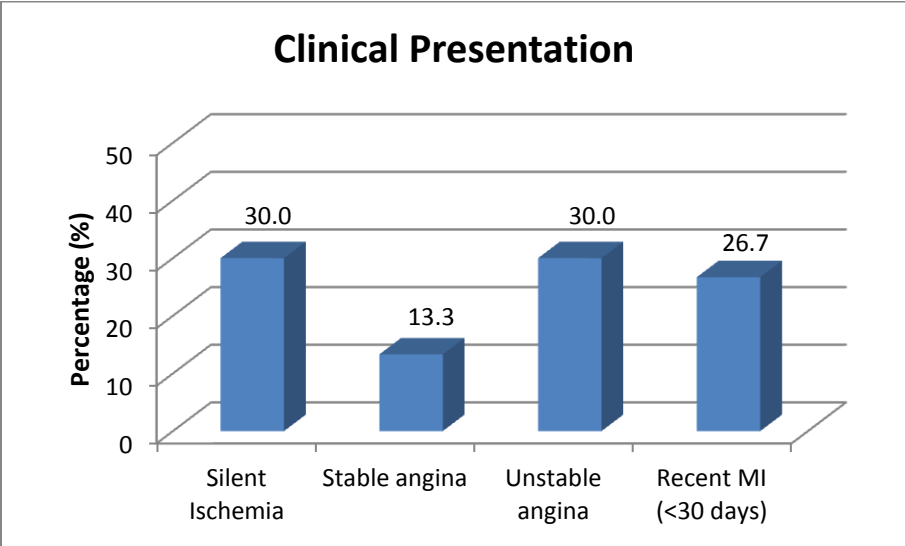

## ❖ References

1. ClinicalTrials.gov – NCT01507519  
<https://clinicaltrials.gov/ct2/show/NCT01507519>
2. CTRI Number: CTRI/2016/11/007475 at <http://ctri.nic.in/Clinicaltrials/pmaindet2.php?trialid=15684&EncHid=&userName=>
3. Dani S, Costa RA, Joshi H, Shah J, Pandya R, Virmani R, Sheiban I, Bhatt S, Abizaid A. First-in-human evaluation of the novel BioMime sirolimus-eluting coronary stent with bioabsorbable polymer for the treatment of single de novo lesions located in native coronary vessels-results from the meriT-1 trial. *EuroIntervention*: 2013 Aug;9 (4):493-500.
4. Costa RA, Abizaid A, Dani S, Joshi H, Wander GS, Hardas S, et al. TCT-212 Efficacy of the novel BioMime sirolimus-eluting stents with a biodegradable polymer in the treatment of de novo coronary lesions: An angiographic subanalysis of the combined meriT-1 and meriT-2 prospective clinical trials. *Journal of the American College of Cardiology*. 2013;62(18 Supplement 1):B68.
5. De Abreu-Silva E, Costa R, Dani S, Lima M, JOSHI H, SHAH J, et al. TCT-578 First-in-human evaluation of a novel sirolimus-eluting stent with a bioabsorbable polymer for the treatment of single, de novo, non-complex coronary lesions. *Journal of the American College of Cardiology*. 2012;60(17 Supplement):B168.
6. Seth A. AS-003 Moving towards biomimicry-development of novel BioMime™ sirolimus eluting coronary stent system. *Journal of the American Journal of Cardiology*. 2011;107(8):1A-2A.
7. Clinical trials department - Meril life sciences. BioMime – A sirolimus-eluting coronary stent system for the treatment of patients with de novo coronary lesions – meriT-1 report. *Interventional Cardiology*, 2011;6(1):39–43.
8. Bhatt S, Gujarathi S, De Benedictis M. Innovative DES technologies from Meril. *Minerva cardioangiologica* 2015;63:441-8.
9. Presented by Roberto Botelho. Outcomes with a thin-strut plla-based sirolimus-eluting stent 1: BioMime , At TCT 2017  
<https://www.tctmd.com/slide/outcomes-thin-strut-lla-based-sirolimus-eluting-stent-1-biomime>